

## Instructions for use of the medical device


SG System Micropipettes for handling of human embryos and oocytes

**Model:** Denudation SG Pipette, Manipulation SG Pipette, Blastocyst SG Pipette, SG Holding Pipette, SG ICSI Pipette, SG Biopsy Pipette, SG Flex Denudation Pipette, SG Flex Manipulation Pipette, SG Flex Blastocyst Pipette.

**Intended Use:** Made from glass and plastic, sterile, single-use pipettes for embryo/oocyte manipulation in vitro with defined inner diameter size.

**Application:** SG System pipettes are used for micromanipulation methods in assisted reproduction. These are glass and plastic sterile pipettes with a defined internal diameter size for single use in the handling of human oocytes and embryos in vitro, vitrification and intracytoplasmic sperm injection (ICSI) or other assisted reproduction methods. They are made of borosilicate glass or plastic (PC) and are designed for single use in healthcare or laboratories of other sectors.

### Labelling description:

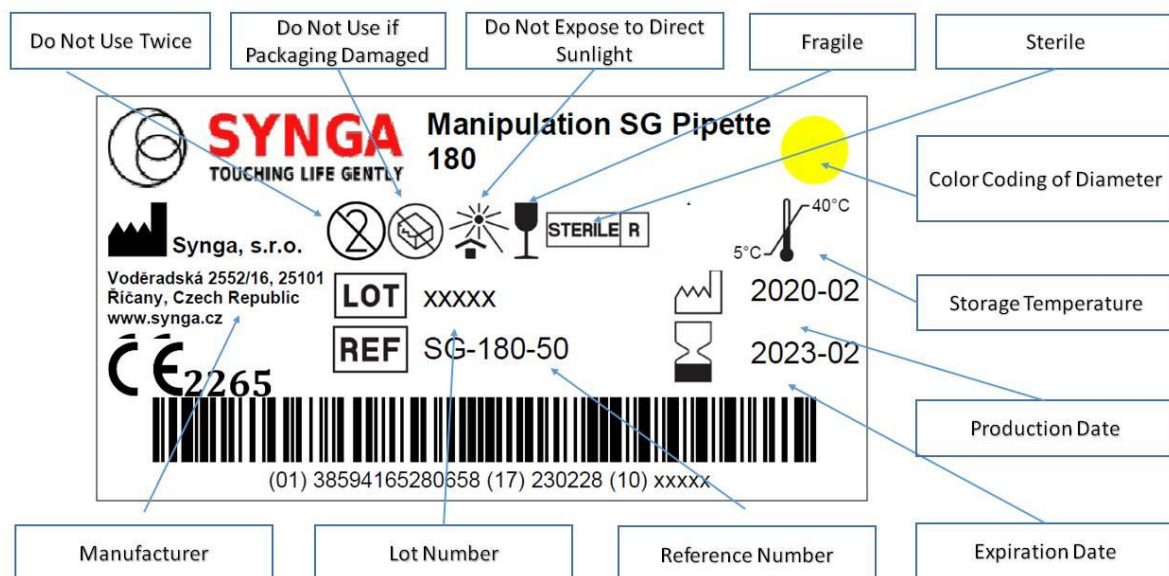

**Vigilance:** In case of an adverse event MD, contact the manufacturer at SYNGA s.r.o., Voděradská 2552/16, 251 01 Říčany u Prahy, Czech Republic, e-mail: [synga@synga.cz](mailto:synga@synga.cz) and follow the instruction of the European Commission for reporting serious adverse events according to paragraph 2 section 1 of Decree No. 62/2015 as amended and MEDDEV 2.12 / 1 rev.8. The respective form is provided by Státní ústav pro kontrolu léčiv – State Institute for Drug Control (SÚKL – [www.sukl.cz](http://www.sukl.cz)).

**Manufacturer:** Synga, s.r.o., Voděradská 2552/16, Říčany, 25101, Czech Republic